

## Contents

---

Area of applicability	3
Important specification in the type code	3
General information	6
Application area	6
Special operating conditions	7
Important information for mounting and maintenance	7
Safe operating mode	9
Potential equalization/Grounding	9
Electrostatic charging (ESD)	10
Instructions for zone 0, zone 0/1 applications	10
Electrical data	11
Mechanical data	11
Thermal data	12
Tensile force on the measuring cable/ rod	14
Installation Control Diagram	15

---

Supplementary documentation:

- Operating Instructions NivoGuide 8100, 3100, 8200
- Quick setup guide NivoGuide 8100, 3100, 8200
- US Certificate of Conformity FM22US0054X (Document ID: 1013252)

Editing status: 2022-06-09



## Area of applicability

These safety instructions apply to the NivoGuide 8100, 3100, 8200 of type series:

- NivoGuide 8100 NG8100.AP\*A/B\*\*1\*\*\* \*\*\*\*\*A/D/N
- NivoGuide 3100 NG3100.AP\*A/B\*\*1\*\*\* \*\*\*\*\*A/D/N
- NivoGuide 8200 NG8200.BP\*A/B\*\*1\*\*0 \*\*\*\*\*A/D/N

With the electronics versions:

- H - Two-wire 4 ... 20 mA/HART
- A - Two-wire 4 ... 20 mA/HART with SIL qualification

According to US Certificate of Conformity FM22US0054X (certificate number on the type label) and for all instruments with safety instruction 1013248.

The classification as well as the respective standards are stated in the US Certificate of Conformity.

Type of protection marking:

- CL I, DIV 1, GP ABCD / CL II, DIV 1, GP EFG / CL III
- CL I, ZN 0, AEx ia IIC T6...T1\*\*\* Ga

## Important specification in the type code

### NivoGuide 8100 NG8100.AP\*A/B\*\*1\*\*\* \*\*\*\*\*A/D/N

Position	Feature	Description
2	Certificate	P FM (IS) CL I, II, III, DIV1, GP ABCDEFG
3	Seal / Second line of defense / Process temperature	A FKM (SHS EPM 70C3 GLT) / without / -40 ... +80 °C
		B EPDM (A+P 70.10-02) / without / -40 ... +80 °C
		D FFKM (Kalrez 6375) / without / -20 ... +150 °C
		F FKM (SHS FPM 70C3 GLT) / without / -40 ... +150 °C
		G FKM (SHS FPM 70C3 GLT) / with / -40 ... +150 °C
		H EPDM (A+P 70.10-02) / without / -40 ... +150 °C
		E Silicone FEP coated (A+P FEP-O-SEAL) / without / -40 ... +150 °C
		K FFKM (Kalrez 6375) / without / -20 ... +200 °C
		L FFKM (Kalrez 6375) / with / -20 ... +200 °C
		M EPDM (A+P 70.10-02) / with / -40 ... +150 °C
		N Silicone FEP coated (A+P FEP-O-SEAL) / with / -40 ... +150 °C
		O Silicone FEP coated (A+P FEP-O-SEAL) / without / -40 ... +80 °C
		P FFKM (Kalrez 6375) / with / -20 ... +150 °C
		Q FKM (SHS EPM 70C3 GLT) / with / -40 ... +80 °C
R EPDM (A+P 70.10-02) / with / -40 ... +80 °C		
S Silicone FEP coated (A+P FEP-O-SEAL) / with / -40 ... +80 °C		

Position		Feature	Description
4	Electronics module	A	Two-wire 4 ... 20 mA/HART
		B	Two-wire 4 ... 20 mA/HART with SIL qualification
5,6	Process fitting	**	Gas-tight threaded connections, pipe connections and industrial flanges acc. to ASME, BS, DIN, EN, GOST, HG/T, JIS, other international, national or industrial standards, regulations or standards, with pressure specifications
8	Version and length of bracket "L" / Material	E	exchangeable rod (ø 8 mm) / 316L
		F	exchangeable rod (ø 12 mm) / 316L
		B	exchangeable cable (ø 2 mm) with gravity weight / 316
		U	exchangeable cable (ø 4 mm) without weight / 316
		A	exchangeable cable (ø 4 mm) with gravity weight / 316
		K	Coax (ø 21.3 mm) with single hole / 316L
		L	Coax (ø 21.3 mm) with multiple hole / 316L
		P	Coax (ø 42.2 mm) with multiple hole / 316L
9	Indicating/adjustment module	0	without
		A	mounted; lid with inspection window
		F	without; lid with inspection window
		B	laterally mounted; double chamber housing, lid with inspection window
10	Length rigid part "L1"	O	without (version with rod)
		Z	L1 = customer-specific (version with cable)
16	Housing	A	Aluminium - single chamber
		D	Aluminium - double chamber
		N	Stainless steel single chamber

## NivoGuide 3100 NG3100.AP\*A/B\*\*1\*\*\* \*\*\*\*\*A/D/N

Position		Feature	Description
2	Certificate	P	FM (IS) CL I, II, III, DIV1, GP ABCDEFG
3	Seal / Process temperature	A	FKM (SHS EPM 70C3 GLT) / -40 ... +80 °C
		F	FKM (SHS FPM 70C3 GLT) / -40 ... +150 °C
		K	FFKM (Kalrez 6375) / -20 ... +200 °C
		B	EPDM (A+P 70.10-02) / -40 ... +80 °C
		H	EPDM (A+P 70.10-02) / -40 ... +150 °C
4	Electronics module	A	Two-wire 4 ... 20 mA/HART
		B	Two-wire 4 ... 20 mA/HART with SIL qualification

Position		Feature	Description
5, 6	Process fitting	**	Gas-tight threaded connections, pipe connections and industrial flanges acc. to ASME, BS, DIN, EN, GOST, HG/T, JIS, other international, national or industrial standards, regulations or standards, with pressure specifications
8	Version and length of bracket "L" / Material	A	exchangeable cable (ø 4 mm) / 316
		F	exchangeable rod (ø 6 mm) / 316
		E	exchangeable steel cable (ø 6 mm with gravity weight / PA coated
		G	exchangeable steel cable (ø 11 mm with gravity weight / PA coated
		H	exchangeable rod (ø 16 mm) / 316L
9	Indicating/adjustment module	0	without
		A	mounted; lid with inspection window
		F	without; lid with inspection window
		B	laterally mounted; double chamber housing, lid with inspection window
16	Housing	A	Aluminium - single chamber
		D	Aluminium - double chamber
		N	Stainless steel single chamber

## NivoGuide 8200 NG8200.BP\*A/B\*\*1\*\*\* \*\*\*\*\*A/D/N

Position		Feature	Description
2	Certificate	P	FM (IS) CL I, II, III, DIV1, GP ABCDEFG
3	Seal / Second line of defense / Process temperature	1	Ceramic-graphite / with / -196 ... +280 °C
		2	Ceramic-graphite / with / -196 ... +450 °C
		3	PEEK-FFKM (Kalrez 6375) / with / -20 ... +250 °C
4	Electronics module	A	Two-wire 4 ... 20 mA/HART
		B	Two-wire 4 ... 20 mA/HART with SIL qualification
5,6	Process fitting	**	Gas-tight threaded connections, pipe connections and industrial flanges acc. to ASME, BS, DIN, EN, GOST, HG/T, JIS, other international, national or industrial standards, regulations or standards, with pressure specifications
8	Version and length of bracket "L" / Material	2	exchangeable cable (ø 2 mm) with centering weight / Duplex (1.4462)
		E	exchangeable rod (ø 8 mm) / 316L
		H	exchangeable rod (ø 16 mm) / 316L
		B	exchangeable cable (ø 2 mm) with gravity weight / 316
		A	exchangeable cable (ø 4 mm) with gravity weight / 316
		L	Coax (ø 21.3 mm) with multiple hole / 316L
		P	Coax (ø 42.2 mm) with multiple hole / 316L

Position		Feature	Description
9	Indicating/adjustment module	0	without
		A	mounted; lid with inspection window
		F	without; lid with inspection window
		B	laterally mounted; double chamber housing, lid with inspection window
16	Housing	A	Aluminium - single chamber
		D	Aluminium - double chamber
		N	Stainless steel single chamber

Multiple listed characteristics according to the dependencies of the device configuration.

In the following, all above mentioned versions are called NivoGuide 8100, 3100, 8200. If parts of these safety instructions refer only to certain versions, then these will be mentioned explicitly with their type code.

## General information

The level measuring instruments NivoGuide 8100, 3100, 8200 as guided radar sensors are used to detect the distance between medium surface and sensor by means of high frequency electromagnetic waves in the GHz range. The electronics uses the running time of the signals reflected by the medium surface to calculate the distance to the medium surface.

The NivoGuide 8100, 3100, 8200 consist of an electronics housing, a process connection element and a sensor, i.e. a measuring cable or a measuring rod. As an option, the display and adjustment module can also be installed in the instrument.

## Application area

The NivoGuide 8100, 3100, 8200 are suitable for use in Class I and Class II in explosive atmospheres of all flammable substances of explosion groups A, B, C, D and dust groups E, F, G, which require Div 1, Div 2 instruments.

The NivoGuide 8100, 3100, 8200 are suitable for applications in class III.

The NivoGuide 8100, 3100, 8200 are suitable for use in explosive atmospheres of all combustible materials of explosion group IIA, IIB, IIC, which require class I, Zone 0, 0/1, 1 AEx ia IIC T6, Ga, Ga/Gb, Gb devices

The NivoGuide 8100, 3100, 8200 with the mechanical fixing element (process fitting) are installed in hazardous areas requiring Div 1, Div 2.

The NivoGuide 8100, 3100, 8200 with the mechanical fixing element (process fitting) are installed in hazardous areas of zone 0 requiring EPL Ga instruments.

The NivoGuide 8100, 3100, 8200 are installed with the mechanical fastening element (process fitting) in the partition wall between zone 1 and zone 0, which separates areas from each other where category EPL Gb or EPL Ga instruments are required.

The NivoGuide 8100, 3100, 8200 with the mechanical fixing element (process fitting) are installed in hazardous areas of zone 1 requiring EPL Gb instruments.

If the NivoGuide 8100, 3100, 8200 are installed and operated in hazardous areas, the general Ex installation regulations, National Electrical Code, further national and regional regulations as well as these safety instructions must be observed.

## Special operating conditions

The following overview is listing all special properties of NivoGuide 8100, 3100, 8200, which make a labelling with the symbol "X" behind the certificate number necessary.

### Electrostatic charging (ESD)

You can find the details in chapter " Electrostatic charging (ESD)" of these safety instructions.

### Ambient temperature

You can find the details in chapter " Thermal data" of these safety instructions.

### Impact and friction sparks

The NivoGuide 8100, 3100, 8200 in light metal versions (e.g. aluminium, titanium, zircon) must be mounted in such a way that sparks from impact and friction between light metals and steel (except stainless steel, if the presence of rust particles can be excluded) cannot occur.

### Non-grounded, metallic parts

The resistance between aluminium housing to metal measuring point identification plate is  $> 10^9$  Ohm.

The capacitance of the metal measuring point identification plate was measured as follows:

Measurement loop identification label	Capacitance
45 x 23 mm (standard)	21 pF
100 x 30 mm	52 pF
73 x 47 mm	61 pF

## Important information for mounting and maintenance

### General instructions

The following requirements must be fulfilled for mounting, electrical installation, setup and maintenance of the instrument:

- The staff must be qualified according the respective tasks
- The staff must be trained in explosion protection
- The staff must be familiar with the relevant valid regulations which are necessary for the safe installation and operation of the device.
- Make sure when working on the instrument (mounting, installation, maintenance) that there is no explosive atmosphere present, the supply circuits should be voltage-free, if possible.
- The instrument has to be mounted according to the manufacturer specifications, the Certificate of Conformity, National Electrical Code and the valid regulations and standards
- Modifications on the instrument can influence the explosion protection and hence the safety, therefore repairs are not permitted to be conducted by the end user
- Modifications must only be carried out by authorized employees
- Use only approved spare parts
- Components for installation and connection not included in the approval documents are only permitted if these correspond technically to the latest standard mentioned on the cover sheet. They must be suitable for the application conditions and have a separate certificate. The special conditions of the components must be noted and if necessary, the components must be integrated in the type test. This applies also to the components already mentioned in the technical description.
- Vessel installations and probable flow must be taken into account

## Cable and wire entries

- The NivoGuide 8100, 3100, 8200 must be connected via suitable cable gland or conduit systems that are in conformity with the requirements of the type of protection and the IP protection or NEMA rating and provided with a separate type approval certificate. When connecting NivoGuide 8100, 3100, 8200 to conduit systems, the corresponding sealing facility must be connected directly to the housing.
- The red thread or/dust covers screwed in when the instruments are shipped (depending on the version) must be removed before setup and replaced by approved cable entries or closing screws suitable for the respective ignition protection type and IP protection or NEMA rating.
- Note type and size of the thread: A label with the respective thread name is in the area of the respective thread
- Threads must have no damages
- Cable entries and closing screws should be mounted correctly and according to the safety instructions of the manufacturer to ensure the specified ignition protection type and IP protection rating or NEMA rating. When using certified or suitable cable glands, closing screws or plug connections, it is absolutely necessary to note the corresponding certificates/documents. Supplied cable entries or closing screws meet these requirements.
- Unused openings must be closed with plugs suitable for the ignition protection type and IP protection or NEMA rating. Supplied plugs meet these requirements.
- Cable or wire entries resp. the closing screws must be tightly screwed into the housing
- The connection cables resp. pipeline sealing facilities must be suitable for the application conditions (e.g. temperature range) of the application
- With surface temperatures  $> 70\text{ °C}$ , the cables must be suitable for the higher application conditions
- The connection cable of NivoGuide 8100, 3100, 8200 has to be wired fix and in such a way that damages can be excluded.

## Mounting

When installing the device, observe the following:

- The instrument must be connected to the grounding system (via the process fitting or an external grounding clamp)
- Mechanical damage on the instrument must be avoided
- Impact and friction sparks are to be avoided
- If the device is used as a partition wall device, the operator must observe the valid applicable installation regulations and ensure a sufficiently tight joint (IP66 or IP67) between the less hazardous area and zone 0 are requiring EPL Ga

## Maintenance

To ensure the functionality of the device, periodic visual inspection is recommended for:

- Secure mounting
- No mechanical damages or corrosion
- Worn or otherwise damaged cables
- No loose connections of the line connections, equipotential bonding connections
- Correct and clearly marked cable connections

The parts of the NivoGuide 8100, 3100, 8200 being in contact with flammable media during operation must be included in the periodic overpressure test of the plant.

## Intrinsic safety "i"

- Observe the valid regulations for the interconnection of intrinsically safe circuits.

- The instrument is only suitable for connection to certified, intrinsically safe instruments
- When connecting a circuit with protection level AEx ib, the device, the sensor meas. system of the device must no more be used in hazardous areas of zone 0.
- When connecting an intrinsically safe instruments with classification mark AEx ia to a circuit with protection level AEx ib, then the classification mark of the instrument changes to AEx ib. After the use as instrument with AEx ib power supply, the instrument must no more be used in circuits with protection level AEx ia
- When connecting an intrinsically safe instrument to an non-intrinsically safe circuit, the instrument must be no longer used in intrinsically safe circuits
- With surface temperatures > 70 °C, the cables must be suitable for the higher application conditions

### **Version with exchangeable cable or rod probe**

Only original cable or rod probes must be mounted to NivoGuide 8100, 3100, 8200. When mounting cable or rod probes, the torques specified in the respective operating instruction manuals must be maintained. The mechanical connection must be ensured.

## **Safe operating mode**

### **General operating conditions**

- Do not operate the instrument outside the electrical, thermal and mechanical specifications of the manufacturer
- Use the instrument only in media against which the wetted parts are sufficiently resistant
- To assess and reduce the explosion risk, the National Electrical Code applicable regulations, rules and standards must be taken into account
- For process pressures outside the standard atmospheric conditions of 80 kPa (0.8 bar) to 110 kPa (1.1 bar) additional requirements can be valid
- Note the relation between process temperature on the sensor/antenna and the permissible ambient temperature on the electronics housing. For permissible temperatures, see the respective temperature tables. See chapter " Thermal data".
- If necessary, a suitable overvoltage arrester can be connected in front of the NivoGuide 8100, 3100, 8200

### **Connection conditions**

The connection cable of NivoGuide 8100, 3100, 8200 has to be wired fix and in such a way that damages can be excluded

If the temperature at the entry parts exceeds 70 °C, temperature-resistant connection cables must be used

## **Potential equalization/Grounding**

- Integrate the instruments into the local potential equalisation, e.g. via the internal or external earth terminal
- The potential equalization terminal must be secured against loosening and twisting
- If grounding of the cable screening is necessary, this must be carried out acc. to the valid standards and regulations
- The intrinsically safe input and the intrinsically safe output circuits are ground-free. The voltage resistance against ground is min. 500 Veff.

## Electrostatic charging (ESD)

In case of instrument versions with electrostatically chargeable plastic parts, the danger of electrostatic charging and discharging must be taken into account!

The following parts can charge and discharge:

- Lacquered housing version or alternative special lacquering
- Plastic housing, plastic housing parts
- Metal housing with inspection window
- Plastic process fittings
- Plastic-coated process fittings and/or plastic-coated sensors
- Connection cable for separate versions
- Type label
- Isolated metallic labels (measuring point identification plate)

Take note in case of danger of electrostatic charges:

- Avoid friction on the surfaces
- Do not dry clean the surfaces

The instruments must be mounted/installed in such a way that the following can be ruled out:

- electrostatic charges during operation, maintenance and cleaning.
- process-related electrostatic charges, e.g. by measuring media flowing past

The warning label indicates danger:

**WARNING - POTENTIAL ELECTROSTATIC  
CHARGING HAZARD - SEE INSTRUCTIONS**

## Instructions for zone 0, zone 0/1 applications

In hazardous areas, the instrument, sensor measuring system in zone 0 should only be operated under atmospheric conditions:

- Temperature: -20 ... +60 °C.
- Pressure: 80 ... 110 kPa (0.8 ... 1.1 bar)
- Air with normal oxygen content, normally 21 %

The operator must ensure that the medium temperature in zone 0 is not higher than 80 % of the self-ignition temperature of the concerned medium (in °C) and does not exceed the max. permissible flange temperature depending on the temperature class. The parts of the sensor which during operation are in contact with flammable products, must be integrated in the periodic overpressure test of the plant.

If no explosive mixtures or additional application conditions are certified or supplementary measures have been taken, then the instruments can be also operated according to the manufacturer specification outside atmospheric conditions.

If there is a risk of dangerous potential differences inside zone 0, then suitable measures for circuits in zone 0 must be taken.

Process fittings between two explosion protection areas require category EPL Ga and less endangered areas must show a tightness in accordance with protection rating IP67 acc. to IEC/EN 60529.

## Electrical data

### NivoGuide 8100, 3100, 8200, single chamber housing, Ex i electronics and connection compartment

Intrinsically safe voltage supply, signal circuit:	
Terminals 1[+], 2[-]	In type of protection intrinsic safety Ex ia IIC
	For connection to a certified, intrinsically safe circuit.
	$U_i = 30 \text{ V}$ $I_i = 131 \text{ mA}$ $P_i = 983 \text{ mW}$
	The effective internal capacitance $C_i$ is negligibly small. The effective internal inductance is $L_i \leq 5 \mu\text{H}$ .

### NivoGuide 8100, 3100, 8200, double chamber housing, Ex i connection compartment

Intrinsically safe voltage supply, signal circuit:	
Terminals 1[+], 2[-]	In type of protection intrinsic safety Ex ia IIC
	For connection to a certified, intrinsically safe circuit.
	$U_i = 30 \text{ V}$ $I_i = 131 \text{ mA}$ $P_i = 983 \text{ mW}$
	The effective internal capacitance $C_i$ is negligibly small. The effective internal inductance is $L_i \leq 10 \mu\text{H}$ .

### NivoGuide 8100, 3100, 8200, single and double chamber housing, Ex i electronics and connection compartment

Intrinsically safe circuit for the display and adjustment module or the interface adapter	
Spring contacts	In type of protection intrinsic safety Ex ia IIC.
	Only for connection to the NivoGuide display and adjustment module.

The circuits of NivoGuide 8100, 3100, 8200 are galvanically separated from ground.

The metallic parts of NivoGuide 8100, 3100, 8200 are electrically connected with the earth terminals.

## Mechanical data

The following mechanical data are valid for all housing and electronics versions.

Mechanical data	
Ground terminal (connection cross-section)	$\geq 4 \text{ mm}^2$
Overvoltage category	See operating instructions NivoGuide 8100, 3100, 8200, chapter " Technical data"

<b>Mechanical data</b>	
Pollution degree	2
<ul style="list-style-type: none"> <li>● Materials</li> <li>● Max. tensile load on the cable or rod probe</li> <li>● Potential connections and electrical separating measures in the instrument</li> <li>● Electromechanical data</li> <li>● Electrical protective measures</li> </ul>	Are described in the operating instructions NivoGuide 8100, 3100, 8200 in chapter " Technical data".

## Thermal data

The following temperature tables are valid for all housing and electronics versions.

If the NivoGuide 8100, 3100, 8200 level transmitters are operated in hazardous areas for EPL Ga, EPL Ga/Gb, EPL Gb and Division 1 applications, the permissible temperature range on the electronics/housings as well as on the sensor (measuring cable, rod) depending on the temperature class can be found in the following table:

Temperature class	Ambient temperature range (Electronics/housing)	Product temperature range on the sensor (measuring cable, rod)
T6	-40 ... +46 °C	-60 ... +80 °C
T5	-40 ... +60 °C	-60 ... +95 °C
T4	-40 ... +60 °C	-60 ... +130 °C
T3	-40 ... +60 °C	-60 ... +195 °C
T2	-40 ... +60 °C	-60 ... +290 °C
T1	-40 ... +60 °C	-60 ... +440 °C

## Low temperature version up to -196 °C

Temperature class	Ambient temperature range (Electronics/housing)	Product temperature range on the sensor (measuring cable, rod)
T6	-40 ... +46 °C	-196 ... +80 °C
T5	-40 ... +60 °C	-196 ... +95 °C
T4	-40 ... +60 °C	-196 ... +130 °C
T3	-40 ... +60 °C	-196 ... +195 °C
T2	-40 ... +60 °C	-196 ... +290 °C
T1	-40 ... +60 °C	-196 ... +440 °C

The sensors (measuring cable, rod) may only be operated in areas for EPL Ga applications if atmospheric conditions are present (pressure of 0.8 ... 1.1 bar).

If there is no explosive atmosphere, the permissible operating temperatures and pressures must be taken from the manufacturer specifications (operating instructions).


If the sensors (measuring cable, measuring rod) are operated at temperatures higher than those listed in the table above, measures must be taken to prevent the risk of ignition from hot surfaces.

The maximum permissible temperature at the electronics/housing must not exceed the values in


the above table.

Temperature derating for process temperatures up to +150 °C, +200 °C, +250 °C, +280 °C and +450 °C


Versions for process temperatures up to +150 °C with metal housing

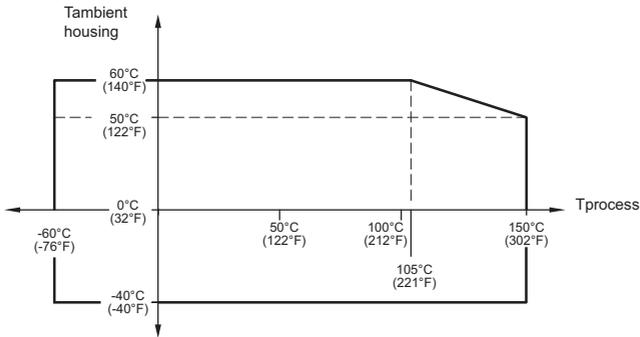


Versions for process temperatures up to +200 °C with metal housing

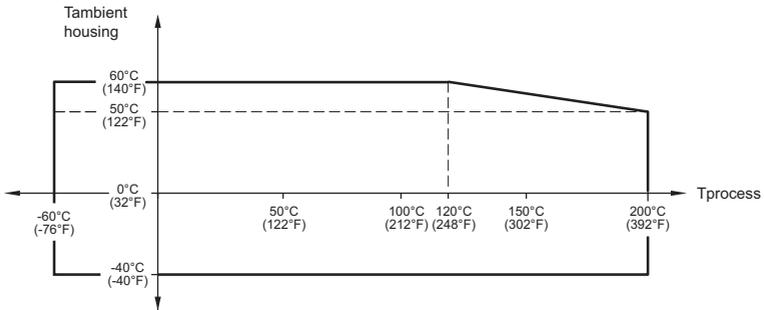


Versions for process temperatures up to +250 °C with metal housing

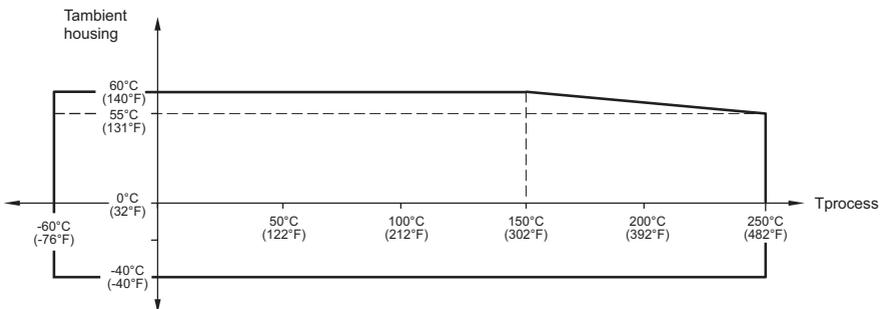

## Versions for process temperatures up to +280 °C with metal housing

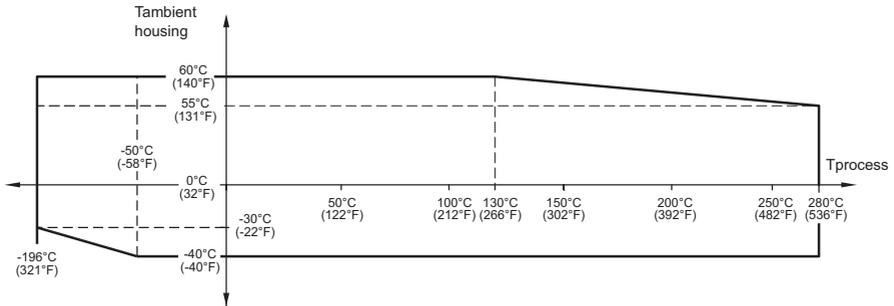

## Versions for process temperatures up to +450 °C with metal housing

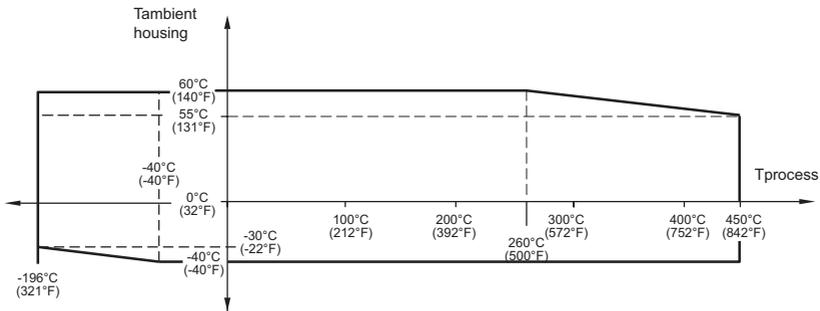

## Tensile force on the measuring cable/ rod

The permissible tensile force is

- NivoGuide 8100
  - Diameter 4 mm: F = 2.5 kN
  - Diameter 2 mm: F = 1.5 kN
- NivoGuide 3100
  - Diameter 4 mm: F = 12 kN
  - Diameter 6 mm coated: F = 8 kN
  - Diameter 6 mm: F = 30 kN
  - Diameter 11 mm coated: F = 30 kN
- NivoGuide 8200
  - Diameter 4 mm: F = 2 kN
  - Exchangeable rod: F = 4.5 kN
- VEGAFLEX 86
  - Diameter 4 mm: F = 2.5 kN
  - Diameter 2 mm: F = 1.5 kN


## Installation Control Diagram

### Installation diagramm

Class I, Division 1, Groups A, B, C, D  
Class II, Division 1, Groups E, F and G  
Class III, Division 1  
or  
Class I, Zone 0, Group IIC  
Class I, Zone 1, Group IIC

Unclassified / Ordinary Location  
or  
Class I, Division 2, Groups A, B, C, D  
or  
Class I, Zone 2, Group IIC

c)

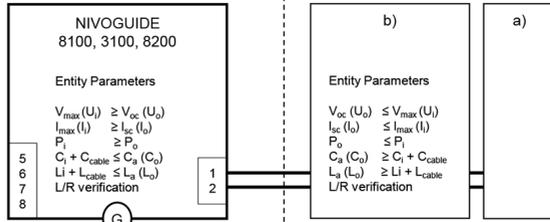

Operation and  
indication circuit(s)

Supply and signal  
circuit

- a) Control Room ( $U_m \leq 253 \text{ V}$ )
- b) Associated Apparatus
- c) Grounding Connection


#### NOTES:

1. The Entity Concept allows the interconnection of suitable approved Intrinsically safe devices with entity parameters not specifically examined in combination as a system when:
  - $U_o$  or  $V_{oc}$  or  $V_i \leq U_i$  or  $V_{\max}$
  - $I_o$  or  $I_{sc}$  or  $I_i \leq I_i$  or  $I_{\max}$
  - $P_o \leq P_i$
  - $C_a$  or  $C_o \geq C_i + C_{\text{cable}}$
  - $L_a$  or  $L_o \geq L_i + L_{\text{cable}}$
2. Control equipment connected to the Associated Apparatus shall not use or generate more than 250  $V_{rms}$  or  $V_{dc}$ .
3. Installation should be in accordance with ANSI/ISA-RP12.06.01 "Intrinsic Safety Wiring Methods for Hazardous (Classified) Locations Instrumentation" and the National Electrical Code (ANSI/NFPA 70 (NEC®). Articles 504 and 505).
4. The configuration of associated Apparatus shall be suitable approved under Entity Concept.
5. Associated Apparatus manufacturer's installation control drawing shall be followed when installing this equipment.
6. The NivoGuide 8100, 3100, 8200 Series are approved for Class I, Zone 0 and Division 1 applications. If connecting [Ex ia]/[AEx ib] Associated Apparatus to the NivoGuide80 Series, the above system is only suitable for Class 1, Zone 1, or Division 2 hazardous (classified) locations, and is not suitable for Class I, Zone 0, or Division 1 hazardous (classified) locations.
7. When cable parameters are unknown, the following may be used: Capacitance = 197 pF/m (60 pF/ft); Inductance = 0.66  $\mu\text{H}/\text{m}$  (0.20  $\mu\text{H}/\text{ft}$ )
8. Resistance between intrinsically safe ground and earth ground must be less than one ohm.
9. No revision to drawing without prior Agency Approval.
10. Warning: Substitution of components may impair suitability for intrinsic safety and hazardous locations.
11. Reference Safety Instructions No. 1013248 for additional information necessary for proper installation.

### Control Drawing NivoGuide 8100, 3100, 8200 adjustment unit; Single chamber housing version

Class I, Division 1, Groups A, B, C, D  
 Class II, Division 1, Groups E, F and G  
 Class III, Division 1  
 or  
 Class I, Zone 0, Group IIC  
 Class I, Zone 1, Group IIC

Unclassified / Ordinary Location  
 or  
 Class I, Division 2, Groups A, B, C, D  
 or  
 Class I, Zone 2, Group IIC

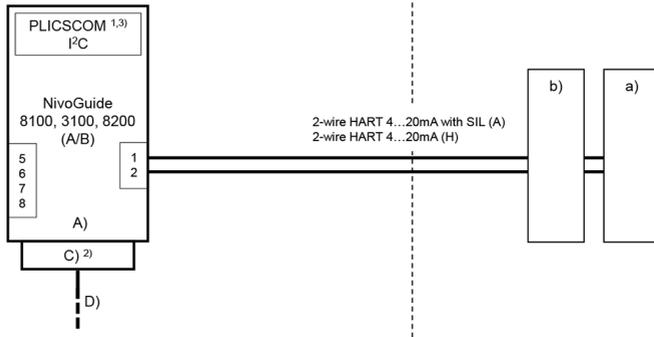

NivoGuide 8100, 3100, 8200 Single chamber housing	$U_i$ (V)	$I_i$ (mA)	$P_i$ (mW)	$C_i$ (μF)	$L_i$ (μH)
Terminals 1, 2	30	131	983	≅ 0	5

- a) Control Room  $U_m \leq 253$  V  
 b) Associated Apparatus with entity parameters IS Barrier  $U_o \leq U_i$ ,  $I_o \leq I_i$ ,  $P_o \leq P_i$ ,  $C_o \geq C_i + C_{cable}$ ,  $L_o \geq L_i + L_{cable}$


- A) Electronics and terminal compartment  
 C) Process fitting  
 D) Rod/cable/ coax probe

<sup>1)</sup> Optional  
<sup>2)</sup> ASME, DIN, G, LA, NPT or TRI-CLAMP industry type flange, with pressure ratings and any type which comply with an international or national standard  
<sup>3)</sup> Only Indicating/adjustment module possible

### Control Drawing NivoGuide 8100, 3100, 8200 and adjustment unit; Double chamber housing

Class I, Division 1, Groups A, B, C, D  
 Class II, Division 1, Groups E, F and G  
 Class III, Division 1  
 or  
 Class I, Zone 0, Group IIC  
 Class I, Zone 1, Group IIC

Unclassified / Ordinary Location  
 or  
 Class I, Division 2, Groups A, B, C, D  
 or  
 Class I, Zone 2, Group IIC

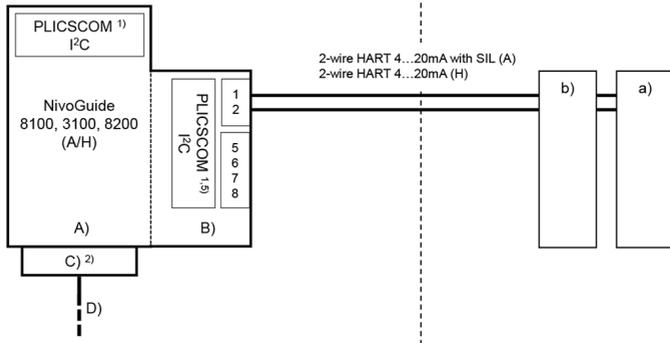

Intrinsically safe parameter of supply and signal circuit

NivoGuide 8100, 3100, 8200 Terminal compartment	U <sub>i</sub> (V)	I <sub>i</sub> (mA)	P <sub>i</sub> (mW)	C <sub>i</sub> (μF)	L <sub>i</sub> (μH)
Terminals 1, 2	30	131	983	≠ 0	5

- a) Control Room U<sub>m</sub> ≤ 253 V  
 b) Associated Apparatus with entity parameters IS Barrier U<sub>o</sub> ≤ U<sub>i</sub>, I<sub>o</sub> ≤ I<sub>i</sub>, P<sub>o</sub> ≤ P<sub>i</sub>, C<sub>o</sub> ≥ C<sub>i</sub> + C<sub>cable</sub>, L<sub>o</sub> ≥ L<sub>i</sub> + L<sub>cable</sub>

- A) Electronics compartment  
 B) Terminal compartment  
 C) Process fitting  
 D) Rod/cable/ coax probe

- <sup>1)</sup> Optional  
<sup>2)</sup> ASME, DIN, G, LA, NPT or TRI-CLAMP industry type flange, with pressure ratings and any type which comply with an international or national standard  
<sup>3)</sup> Only Indicating/adjustment module possible





Printing date:

All statements concerning scope of delivery, application, practical use and operating conditions of the sensors and processing systems correspond to the information available at the time of printing.  
Subject to change without prior notice

**Technical support**

Please contact your local sales partner (address at [www.uwt.de](http://www.uwt.de)). Otherwise please contact us:

UWT GmbH  
Westendstraße 5  
87488 Betzigau  
Germany

Phone + 49 (0) 831 57 123 42  
[info@uwtgroup.com](mailto:info@uwtgroup.com)  
[www.uwtgroup.com](http://www.uwtgroup.com)

1013248-EN-220921